



CryoTDS – 100H2 can Analyze Hydrogen in Plating Films with a very Simple Operating Procedure


Thermal Desorption Spectrometer CryoTDS – 100H2

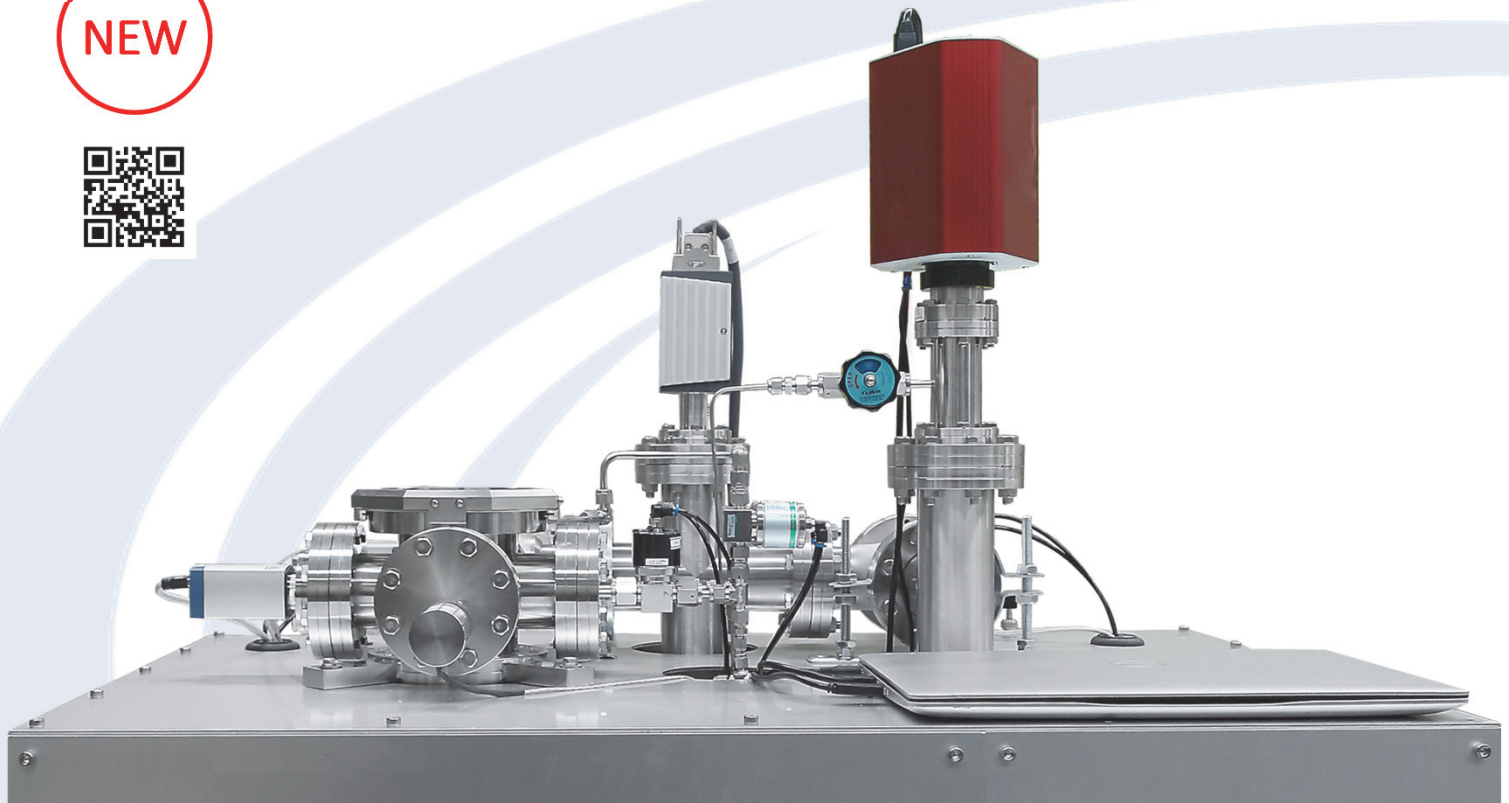

Electroless Ni plating (5 μ m)

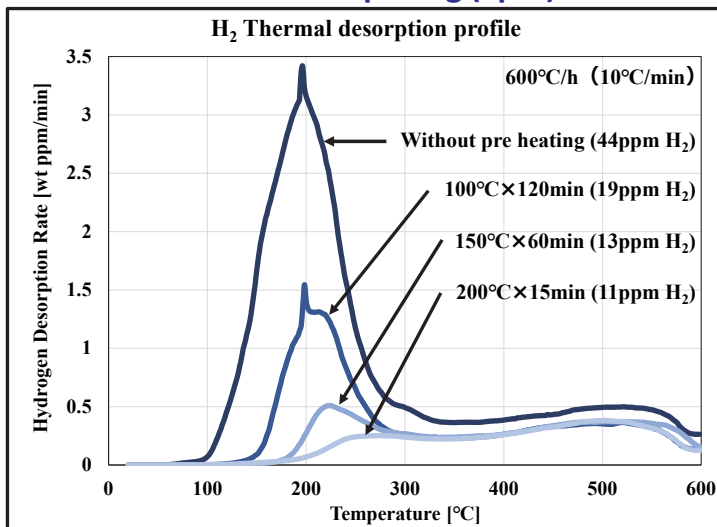

Electro Ni plating (5 μ m)

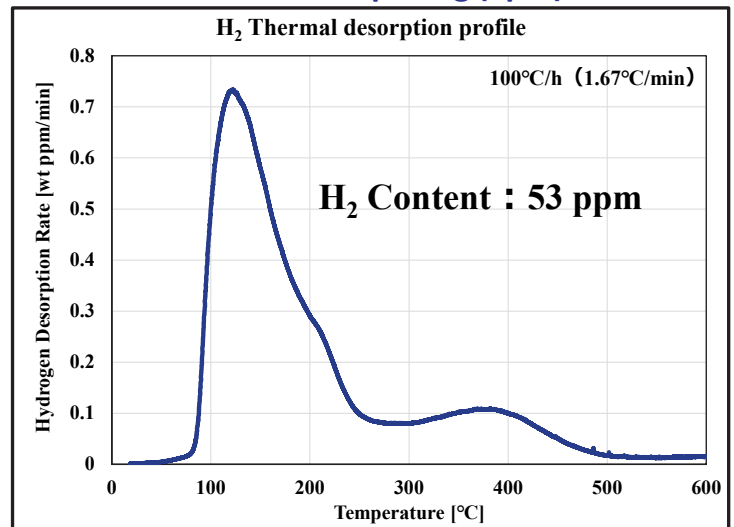

The answer for diffusible hydrogen quantitation is CryoTDS – 100H2.
A low-temperature option will be released soon.